


Specification Curve

Difference in alpha
power change from pre-
to post-intervention
between conditions (%)

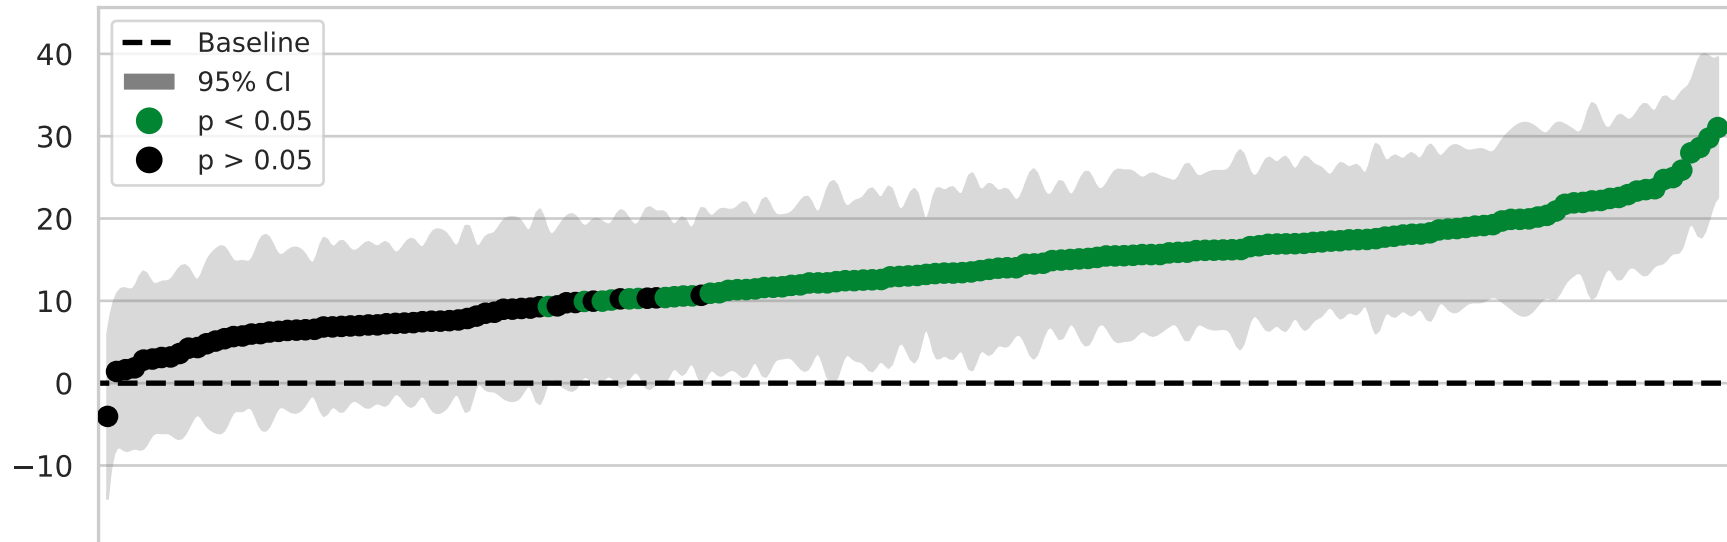

Alpha power
electrode

P4
P3
O2
O1
Pz

Stimulation
frequency (Hz)

11
10
9
IAF

Resampling (Hz)

512
500
250

Analysis
software

EEGLab
FieldTrip
MNE

