

QA File Parameter

Patient Name : XXXXXXXXXX
 Patient ID : XXXXXXXXXX
 Plan Date : 2/5/2020
 SSD :
 SDD :
 Depth :
 Energy : 6X
 Angle :

Absolute Dose Comparison

Difference (%) : 2.0
 Distance (mm) : 2.0
 Threshold (%) : 20.0
 Meas Uncertainty : No
 Use Global % : No

Summary (GC Analysis)

Total Points : 567
 Passed : 512
 Failed : 55
 % Passed : 90.3
 *GC/Gamma is using 3D Mode

Dose Values in cGy


	CAX	Norm	Sel	Max
ArcCHECK		91.04	49.02	91.04
Plan	52.69	93.00	53.25	93.26
ArcCHECK		-1.97	-4.23	-2.22
-Plan				
% Diff		-2.11	-7.95	-2.39
Coords (y,x) cm	0,0	1,19.5	0,-0.5	

Notes


bst1
 pelvis
 SLC

Reviewed By :

ArcCHECK

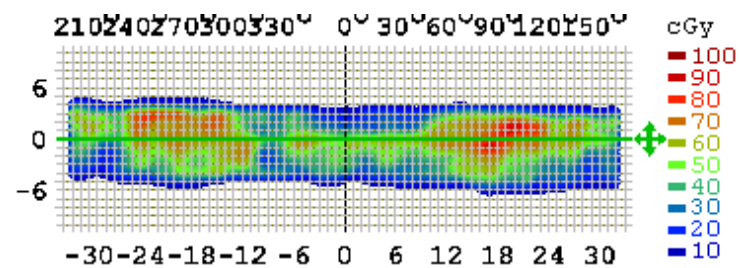

Plan

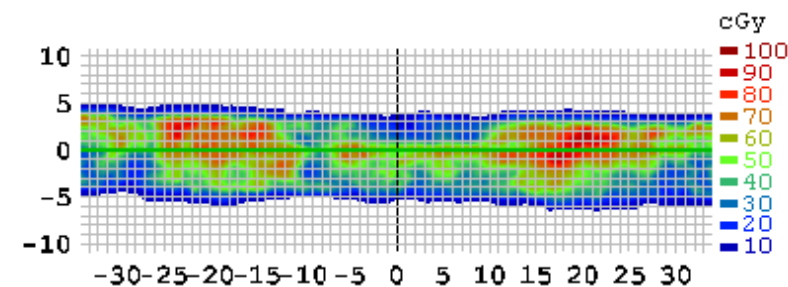

ArcCHECK-Plan

